



Lower Extremity Sail Measurement Form

CJ Socket Technologies

100 Cummings Center • Suite 207H • Beverly, MA 01915

Tel: 978-922-0413 • Fax: 978-922-0277

CJSocket@gmail.com • www.CJSocket.com

Company Name: _____

Prosthetist Name: _____

Purchase Order #: _____ Phone: _____ Fax: _____

Email: _____

Shipping Address: _____

City: _____ State: _____ ZIP code: _____

Billing Address (if different): _____

City: _____ State: _____ ZIP code: _____

Shipping: Priority Mail 2-3 Day (Standard) Next Day Other: _____

Patient Height: _____, Patient Weight: _____, Amputated Side: Left Right

K Level: 1 2 3 4

Material Color: Black Coyote (Brown) Heavy Duty Fabric (Black Only)

Closure Options: Standard (1:1) Closure, 1.5" Velcro Attached to Batten
 (2:1) Closure, 1.5" Loops Attached to Batten. **(Customer supplies Velcro Straps)****
 (2:1) Closure, 1" Loops Attached to Batten, 1" Pressure Buckles with Dacron Strap (No Velcro)

Other Options: Proximal Arc (for very Conical or Flexed Residual Limbs, Degrees of Socket Flexion _____ (Required))
 Darts Sewn into Sail (for Irregular Shaped Residual Limbs) Dart Measurements (H" x W"): _____
 This is a Replacement Sail for an existing socket, No Holes Needed
 OPEN FLAP Design – Medial Side of Sail Will Not Have Attachment Holes – Secured by Closure Choice Above
 **CJ Socket to Make Dacron-backed Velcro Straps (to be used with (2:1) Closure, 1.5" Loops Attached to Batten)

Special Instructions: _____


Internal use only

Serial # _____

Date in _____

Date out _____

TFB _____

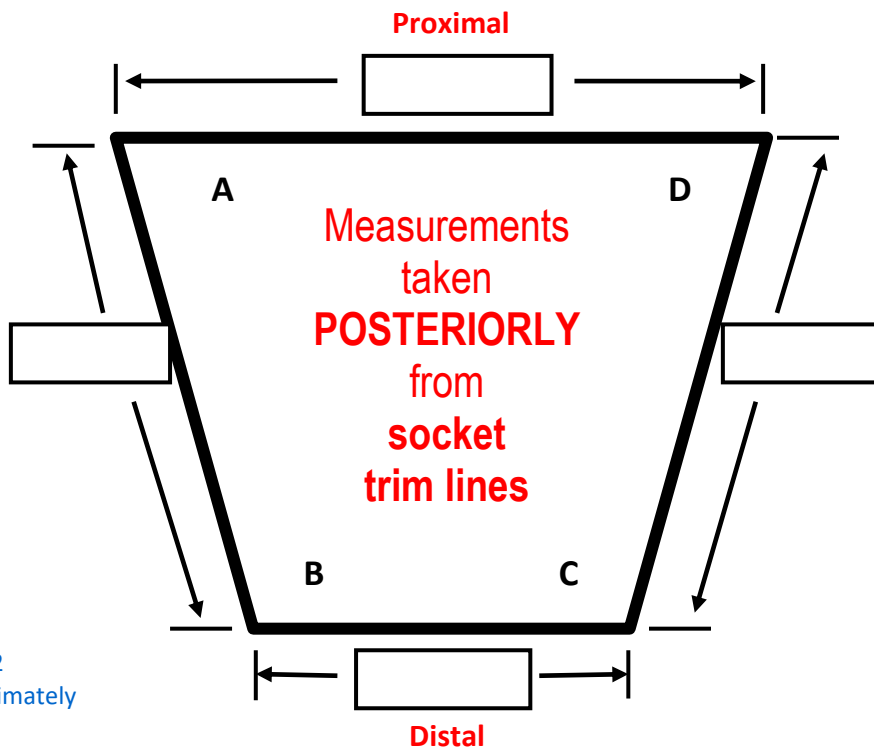

Measurements is:

Inches
 CM

Indicate:
 Medial or Lateral

Indicate:
 Medial or Lateral

Standard attachment hardware includes 8-32 Chicago screws approximately 2" on center.